



ANCHOR
VZV PCR KIT

Instructions for Use
ANCHOR VZV PCR Kit




Quantitative or Qualitative
real-time PCR Kit
for *in vitro* diagnostic use

IVD For *in vitro* diagnostic use


REF A1000

 100

 A1010-EN, 2025-06-17

QG A1011-EN, 2025-06-17

 -30°C to -15°C

 **ANCHOR** Diagnostics GmbH
Grandweg 64
D-22529 Hamburg

compatible with

QuantStudio 5 (Applied Biosystems)

LightCycler 480 II (Roche)

cobas z 480 Analyzer (Roche)

CFX96 (Bio-Rad)

Rotor-Gene Q (QIAGEN)

Mic qPCR (Bio Molecular Systems)

1	▶ Contents	
2	Intended Use.....	6
3	Product Description.....	6
4	Kit Components.....	6
5	Storage and Stability.....	7
6	Material Required but Not Provided.....	8
7	Limitations.....	8
8	Warnings and Precautions	9
9	Workflow	10
9.1	Sample Preparation.....	10
9.1.1	Sample Matrix.....	10
9.1.2	Sample Preparation.....	11
9.1.3	Internal Control.....	12
9.2	PCR Preparation	13
9.2.1	Master Mix Set-Up.....	13
9.2.2	PCR Reaction Set-Up	15
9.3	PCR Cycler Configuration	16
9.3.1	General PCR Cycler Settings	16
9.3.2	Specific PCR Cycler Settings	17
9.4	Data Analysis	19
9.4.1	Qualitative Analysis.....	21
9.4.2	Quantitative Analysis.....	22
10	Performance Data.....	23
10.1	Analytical Performance.....	23
10.1.1	Sensitivity.....	23
10.1.2	Linearity.....	24
10.1.3	Specificity.....	25
10.1.4	Precision	27
10.2	Clinical Performance.....	28
11	Quality Control.....	29
12	Technical Assistance & Contact Information	29
13	Symbols.....	30

2 ▶ Intended Use

The ANCHOR VZV PCR Kit is an *in vitro* nucleic amplification test based on real-time PCR technology for the quantitative or qualitative detection of VZV DNA, isolated from human EDTA plasma, cerebrospinal fluid or cutaneous/mucocutaneous lesions.

The product is intended to be used by professional operators, such as technicians and physicians who are trained in molecular biological techniques.

3 ▶ Product Description

The Kit constitutes a ready-to-use system for the amplification, detection and quantitation of VZV-specific nucleic acids.

In addition, a heterologous amplification system (Internal Control) is included to supervise the success of the sample extraction procedure and to identify possible inhibition of the amplification reaction.

Probes linked to distinguishable fluorescent dyes enable the parallel detection of VZV specific nucleic acids and the Internal Control in two corresponding detector channels of the real-time PCR instrument.

The Quantitation Standards QS1-4 VZV contain defined concentrations of artificial DNA bearing the VZV target sequence. They can be used individually or as a whole set together with the Negative Control DNA to monitor the integrity of the analyte-specific reagents of the kit and the proper performance of the reaction. When the Quantitation Standards QS1-4 VZV are used as a whole set, they allow to quantitate the VZV DNA present in a test sample.

4 ▶ Kit Components

Master A and Master B reagents contain all necessary components (PCR buffer, Polymerase, magnesium ions, dNTPs, primers, and probes) to allow PCR-mediated amplification and target detection of VZV specific DNA and Internal Control in one reaction setup.

The Quantitation Standards QS1-4 VZV and NC (Negative Control) DNA are supplied with the IC (Internal Control) DNA already incorporated (see also section 9.2.1 Master Mix Set-Up).

The reagents provided with the kit allow the preparation of 100 reactions.

Kit component	Mat. no.	No. of vials	Quantity	Ingredients
Master A VZV	A1001	4 vials	4x 125 µL	Buffer, bovine serum albumin, polymerase
Master B VZV	A1002	4 vials	4x 125 µL	Buffer, salt, nucleotides, target- and IC-specific oligonucleotides
IC DNA	AD00020	1 vial	1000 µL	Buffer, IC-specific synthetic polynucleotide
QS1-4 VZV*	A1003-1/2/3/4	1 vial each	4x 200 µL	Buffer, target- and IC-specific synthetic polynucleotide
NC DNA*	AD00021	1 vial	200 µL	Buffer, IC-specific synthetic polynucleotide

* INTERNAL CONTROL INSIDE !

5 ▶ Storage and Stability

- The ANCHOR VZV PCR Kit is shipped on dry ice and should be stored at -30 to -15°C upon receipt.
- The components are stable until the expiration date stated on the label.
- Do not use components of the kit that have passed their expiration date.
- Store VZV DNA-positive and/or potentially positive material separated from the kit.
- Repeated thawing and freezing of the Master reagents of > 3x should be avoided, as this may reduce the assay performance. For the Quantitation Standards QS1-4 VZV, the NC DNA and the IC DNA, thawing and freezing cycles up to 4x are allowed.
- Due to the components used it might be possible that Master vials do not always freeze completely after initial thawing. This is not a matter of concern and does not influence the stability or performance of the assay.
- If the reagents are to be used only intermittently, they should be frozen in aliquots. Label aliquots clear and unambiguously to avoid a mix-up of reagents.
- During PCR set up the reagents should be kept cooled at +2 to +8°C – use cooling block.
- Do not store components more than 3 h at +2 to +8°C.
- Protect all reagents from extensive light exposure.

6 ▶ Material Required but Not Provided

- Nucleic acid purification system
- Real-time PCR instrument
- Appropriate PCR reaction vessels and related accessories
- Cooling block (for reaction setup)
- Benchtop centrifuge (rotor holding 2 mL reaction tubes)
- Vortex mixer
- Pipettes (variable volume)
- Single-use pipette filter tips
- 1.5 mL or 2 mL reaction tubes (for Master mix set-up)
- Single-use gloves (powder-free)

Use all materials and equipment according to the manufacturer's instructions. Maintain and calibrate the equipment as recommended.

7 ▶ Limitations

- Strict compliance with the user manual is required for optimal PCR results.
- Any diagnostic result generated must be interpreted in conjunction with other clinical and/or laboratory findings.
- The presence of PCR inhibitors may cause invalid results.
- Occurrence of mutations within the target region might result in a reduced sensitivity, false quantitation or a complete detection failure.
- Following good laboratory practices is crucial for the successful usage of the product.
- Appropriate handling of the reagents is essential to avoid contaminations or impurities.

8 ▶ Warnings and Precautions

- For *in vitro* diagnostic use.
- Use of this product is limited to personnel specially instructed and trained in the techniques of real-time PCR and *in vitro* diagnostic procedures.
- Specimens should always be treated as potentially infectious and/or biohazardous material in accordance with safe laboratory procedures.
- Wear protective single-use gloves, a laboratory coat and eye protection when handling specimens or kit components.
- Avoid microbial and nuclease (DNase/RNase) contamination of the specimen and the components of the kit.
- Always use DNase/RNase-free single-use pipette tips with aerosol barriers.
- Use separated working areas for (1) specimen preparation, (2) PCR reaction set-up and (3) amplification/detection activities.
- Dedicate supplies and equipment to the separate working areas and do not move them from one area to another.
- Do not open the reaction tubes/plates post amplification, to avoid contamination with amplicons.
- Additional controls may be tested according to guidelines or requirements of local, state and/or federal regulations or accrediting organizations.
- Discard sample and assay waste according to your local safety regulations.

9 ▶ Workflow

9.1 ▶ Sample Preparation

9.1.1 ▶ Sample Matrix

The recommended patient sample matrices for sample preparation input are

- human EDTA plasma
- cerebrospinal fluid
- cutaneous and mucocutaneous lesions.

The blood draw should be done using commercially available standard blood collection systems for EDTA-plasma (e.g. Sarstedt, Becton Dickinson, Greiner or equivalent). Tube contents should be mixed directly after sample collection according to manufacturer's instructions. For separation of EDTA-plasma, whole blood should be centrifuged according to the instructions provided by the manufacturer of the collection system within 24 hours after collection.

If a sample is not directly processed, store samples according to manufacturer's instructions (Collection Tube, Transport Tube, Sample Preparation Kit) before use.

Storage recommendations:

Although several studies reported a relative stability of herpes viruses and their nucleic acids (Hasan et al. & Smit et al.) - if not specified by related manufacturer's instructions - storage of clinical samples under refrigerated conditions (+2°C to +8°C) should not exceed 3-4 days.

For long term storage clinical materials and purified nucleic acids should be frozen (at least -30°C to -15°C).

Short-Term Stability of Pathogen-Specific Nucleic Acid Targets in Clinical Samples

Mohammad R. Hasan, Rusung Tan, Ghada N. Al-Rawahi, Eva Thomas, Peter Tilley

Journal of Clinical Microbiology Nov 2012, 50 (12) 4147-4150

*Comparison of collection methods for molecular detection of α -herpes viruses and *Treponema pallidum*, including evaluation of critical transportation conditions.*

Pieter W. Smit, Titia Heijman, Meriem el Abdallaoui, Sylvia M. Bruisten Heliyon 5 (2019) e01522

9.1.2 ▶ Sample Preparation

Purified DNA is the sample input material for the ANCHOR VZV PCR Kit. It has to be ensured that the chosen nucleic acid purification method is compatible with real-Time PCR technology. The extraction has to be executed according to the manufacturer's instructions.

The diagnostic applicability of the ANCHOR VZV PCR Kit has been shown using the following sample preparation platforms:

Sample Preparation Platforms

NucliSENS® easyMag® System (bioMérieux)

EMAG® (bioMérieux)

EZ1 Advanced XL / EZ2 Connect (QIAGEN)

QIAcube Connect (QIAGEN)

QIASymphony® SP (QIAGEN)

MagNA Pure 96 System (Roche)

MagNA Pure Compact (Roche)


Maxwell® 16 / RSC Instruments (Promega)


KingFisher Systems (Thermo Fisher Scientific)

SEEPREP32™ (Seegene)

GenoXtract® (Hain Lifescience)

PLEASE NOTE


 If sample eluates are not directly used for PCR analysis, store eluates at -30 to -15°C. In case of using eluates repeatedly, avoid frequent thaw/freeze cycles (not more than 3 cycles).

 Eluates should be labeled clearly and unambiguously to avoid a mix-up of samples.

9.1.3 ▶ Internal Control

The Internal Control DNA provided with the ANCHOR VZV PCR Kit should be co-purified with the nucleic acid of interest to monitor sample preparation efficiency and quality.

PLEASE NOTE

 The Internal Control DNA **MUST NOT** be added directly to the clinical sample.

Always add the Internal Control DNA after lysis buffer has been added to the sample.


The required volume of Internal Control DNA per sample purification is defined by the chosen elution buffer volume.

Ten percent of the elution buffer volume used should be added to the sample/lysis mixture.

Examples:

- Elution buffer per sample: 200 µL → IC DNA volume: 20 µL
- Elution buffer per sample: 60 µL → IC DNA volume: 6 µL

PLEASE NOTE


 Secure the elimination of residual ethanol before elution of nucleic acids. Ethanol may inhibit the amplification process.

If no co-purification of the Internal Control is planned and the IC DNA should be used only as an inhibition control of the reaction, either the amount of IC related to the used elution volume could be added to each eluate or 1.5 µL of the IC DNA per reaction should be added to the master mix (see section 9.2.1 Master Mix Set-Up).

9.2 ▶ PCR Preparation

9.2.1 ▶ Master Mix Set-Up

PLEASE NOTE

 Consider configuring the run settings of the PCR cycler software to have the instrument ready before starting the PCR reaction preparation (Refer to section 9.3 PCR Cycler Configuration).

Prepare the Master Mix step by step:

- Thoroughly thaw Master components A and B.
- Mix Master A and B by gentle pipetting or short pulse-vortexing.
- Spin Master A and B shortly with a benchtop centrifuge to remove residual droplets from tube lids.
- According to your preferred workflow follow one of the pipette schemes below to mix Master A and B using a 1.5 mL or 2 mL reaction tube:

IC DNA present in sample eluates – NO IC DNA added to Master Mix preparation:

Number of reactions	1	10(+1)*	N**
Master A VZV	5 µL (X)	55 µL	Y µL
Master B VZV	5 µL (X)	55 µL	Y µL
Volume Master Mix	10 µL	110 µL	Z µL

*10 reactions + 10%

** See formula on next page

IC DNA to be used as inhibition control only – IC DNA added to Master Mix preparation:

Number of reactions	1	10(+1)*	N**
Master A VZV	5 µL (X)	55 µL	Y µL
Master B VZV	5 µL (X)	55 µL	Y µL
IC DNA	1.5 µL (X)	16.5 µL	Y µL
Volume Master Mix	11.5 µL	126.5 µL	Z µL

*10 reactions + 10%

** See formula on next page

PLEASE NOTE

i We recommend calculating for an additional volume of at least 10% to compensate potential loss during pipetting. The needed volume will be calculated by using the following formula:

$$** N \times X \mu L \times 1,1 = Y$$

N = Number of reactions

X = Volume of component per reaction

Y = Total volume of component

Z = Total volume of Master Mix

- Mix prepared Master Mix by gentle and short pulse-vortexing.
- Spin Master Mix shortly with a benchtop centrifuge to remove residual droplets from tube lids.

i It is recommended to test all 4 Quantitation Standards and the Negative Control at least once in each PCR run. For qualitative analyses, the use of QS3 VZV as Positive Control is recommended. For further information, see also chapters 9.4.1 and 9.4.2, respectively.

i Quantitation Standards QS1-4 VZV and the Negative Control DNA already contain the IC DNA in a ready-to-use concentration. No addition of IC necessary!

If you want to use a Master Mix preparation with added IC DNA (as inhibition control) in combination with the QS1-4 and NC DNA, be aware that the IC signal of the controls will slightly shift towards a lower CT value in comparison to the IC signal of the controls using a Master mix without additional IC.

9.2.2 ▶ PCR Reaction Set-Up

PLEASE NOTE

i Always use a cooling block for the preparation of the PCR reaction mix.

Prepare the Reaction Mix step by step:

- If previously stored frozen, thaw eluates containing nucleic acid (and IC DNA) thoroughly.
- Mix eluates by gentle pipetting or brief pulse-vortexing.
- Spin eluates shortly with a benchtop centrifuge to remove residual droplets from tube lids.
- Pipette **10 µL of Master Mix** (see section 9.2.1 Master Mix Set-Up) into suitable reaction vessels for PCR analysis. This is also valid for Master Mix spiked with IC DNA.
- Add **15 µL of eluate** or control (Quantitation Standards QS1-4 VZV or Negative Control DNA). **Mix well by repeated up and down pipetting!**
- Close reaction vessels securely with the appropriate sealing system.
- Immediately transfer closed and ready-to-use reaction vessels to the real-time PCR instrument. Avoid any delays!

PLEASE NOTE

i Carefully handle reaction vessels during transfer to avoid mixing up samples.

i Complete mixing of Master Mix reagents with a sample or control during reaction set up should be unconditionally secured by repeated up and down pipetting!
This is essential for achieving optimal amplification curve performance.

Master Mix	Eluate / Control	Reaction Mix
10 µL	15 µL	25 µL

9.3 ▶ PCR Cyclers Configuration

The ANCHOR VZV PCR Kit has been evaluated in combination with the following different PCR Cycler platforms:

PCR Cycler Platform	Run Time
QuantStudio 5 (Applied Biosystems)	≈ 28 min.
LightCycler 480 II (Roche)	≈ 30 min.
Cobas z 480 Analyzer (Roche)	≈ 30 min.
CFX96 (Bio-Rad)	≈ 33 min.
Rotor-Gene Q (QIAGEN)	≈ 39 min.
Mic qPCR (Bio Molecular Systems)	≈ 34 min.

The listed run times for the different instruments are effectively measured durations and can differ from what is displayed on the graphical user interface of the individual instrument software. For basic information concerning set-up and programming of the respective real-time PCR instrument, refer to the instrument-specific manual.

9.3.1 ▶ General PCR Cycler Settings

Temperature cycling profile for **QuantStudio 5, LightCycler 480 II (Roche), Cobas z 480 Analyzer, CFX96 and Rotor-Gene Q:**

Cycling	95°C	1 sec	x 40
	65°C *	2 sec	
	72°C	1 sec	

* Fluorescence acquisition for VZV and IC

Temperature cycling profile for **Mic qPCR:**

Cycling	95°C	1 sec	x 40
	63°C *	2 sec	
	72°C	1 sec	

* Fluorescence acquisition for VZV and IC

Reaction Volume: 25 µL

9.3.2 ▶ Specific PCR Cycler Settings

The following tables contain PCR cycler-specific recommendations for the basic configuration of the run settings.

For additional information regarding the cycler settings recommended plastics, color compensation, gain optimization settings, etc. do not hesitate to contact us directly (see section 12 Technical Assistance & Contact Information).

QuantStudio™ 5		
Target	VZV	IC
Detection	FAM	HEX
Run Settings		
<ul style="list-style-type: none"> Block Type: 96-Well 0.1-mL Block Experiment Type: Standard Curve Chemistry: TaqMan® Reagents Run Mode: Fast Plate attributes: Passive Reference - None 		
Consumables:		
<ul style="list-style-type: none"> 96-Well Fast Thermal Cycling Plates (Life Technologies Mat.No. 4346907) MicroAmp™ Optical Adhesive Film (Life Technologies Mat. No. 4311971) 		

LightCycler® 480 II and cobas z 480 Analyzer		
Target	VZV	IC
Detection	465/510	LightCycler 480 II: 533/580 cobas z 480 Analyzer: 540/580
Run Settings:		
<ul style="list-style-type: none"> Block size: 96 If clear plates are used, the sensor of the LightCycler® has to be disabled by selecting the Clear Plates option in the software before the run is started. 		
Consumables:		
<ul style="list-style-type: none"> LC480 Multiwell Plate 96, white (Roche Mat. No. 04729692001) LC480 Multiwell Plate 96, clear (Roche Mat. No. 05102413001) LC480 Sealing Foil (Roche Mat. No. 04729757001) 		

Bio-Rad CFX96		
Target	VZV	IC
Detection	FAM	HEX
Consumables: <ul style="list-style-type: none"> ▪ Hard Shell 96-well PCR Plate, white (Mat. No. HSP9655) ▪ Optical flat 8 Cap Strip for 0.2mL (Mat. No. TCS0803) ▪ 0.2 mL 8-Tube PCR Strips without Caps, low profile, white (Bio-Rad Mat. No. TLS 0851) ▪ 8-strip optical clear flat caps (Sarstedt Mat. No. 65.1998.400) 		

Rotor-Gene Q		
Target	VZV	IC
Detection	Green	Yellow
Run Settings <ul style="list-style-type: none"> ▪ Use 72-Well Rotor ▪ Perform Auto-Gain optimization before 1st acquisition. 		
Consumables: <ul style="list-style-type: none"> ▪ Strip Tubes and Caps, 0.1 mL (QIAGEN Mat. No. 981103) 		

Mic qPCR		
Target	VZV	IC
Detection	Green	Yellow
Run Settings <ul style="list-style-type: none"> ▪ Temperature Control: Standard TAQ 		
Consumables: <ul style="list-style-type: none"> ▪ Mic Tubes and Caps (Mat. No. 68MIC-60653) 		

When preferring a quantitative analysis of the clinical samples, the Quantitation Standards QS1-4 VZV must be labeled as standards within the instrument software and assigned with their appropriate concentrations.

Quantitation Standard	Concentration [copies/ μ L]
QS1 VZV	10,000
QS2 VZV	1,000
QS3 VZV	100
QS4 VZV	10

9.4 ▶ Data Analysis

The following table contains cycler-specific references for the configuration of analysis settings. They could serve as an initial orientation. Depending on local cycler- and workflow-related differences adaptations might be necessary.

For additional information concerning data analysis, refer to the instrument-specific manual of the respective real-time PCR instrument or contact us (see section 12 Technical Assistance & Contact Information).

QuantStudio™ 5
Analysis Settings (all channels): <ul style="list-style-type: none"> ▪ Plot Type: ΔRn vs Cycle ▪ Graph Type: Linear ▪ Baseline Start/End: 3/15 ▪ Threshold: <ul style="list-style-type: none"> - FAM 250,000 - HEX 50,000

LightCycler® 480 II and cobas z 480 Analyzer
Analysis Settings: <ul style="list-style-type: none"> ▪ Abs Quant/Fit Points ▪ Color Comp (off) ▪ Mean ▪ High Confidence ▪ Threshold <ul style="list-style-type: none"> - 465/510: 0.6 - 533/580: 1.4

Bio-Rad CFX96
Analysis Settings (all channels): <ul style="list-style-type: none"> ▪ Baseline Subtracted Curve Fit ▪ C(t) Determination Mode: Single Threshold ▪ Baseline Threshold: <ul style="list-style-type: none"> - Baseline Cycles: Auto Calculated - Single Threshold <ul style="list-style-type: none"> - FAM: 1,000 - HEX: 250

Rotor-Gene Q

Analysis Settings (all channels):

- Quantitation
- Linear Scale
- Dynamic Tube ON
- Threshold:
 - Green: 0.05
 - Yellow: 0.08

Mic qPCR

Analysis Settings (all channels):

- Graph Type: Linear
- Method: Dynamic
- Ignore Cycles Before: 3
- Threshold Start: 1
- Exclusion: None
- Threshold Level:
 - Green: 1.30
 - Yellow: 1.70

9.4.1 ► Qualitative Analysis

For a valid run and as a prerequisite for the interpretation of the individual clinical sample results, the following requirements have to be met by the included kit controls:

Channel/Target	VZV	IC
QS3 VZV ¹	+	+
NC DNA	-	+

¹ It is recommended to use QS3 VZV as Positive Control, but the criteria also apply to QS4 VZV. QS1-2 VZV are excluded from these criteria. The presence of high concentrated artificial nucleic acids in those Quantitation Standards can result in a competitive inhibition of the IC amplification.

If one of the conditions has failed, result interpretation of clinical sample results might be flawed. In case of kit control failure, it is recommended to repeat the PCR run.

In case of a valid run, the following result interpretation can be made:

Qual. result	VZV	IC
VZV DNA Positive	+	+/-
VZV DNA Negative	-	+
Invalid	-	-

A positive result for VZV DNA does not necessarily require a positive signal for the IC since high concentrations of the respective target nucleic acid can result in a competitive inhibition of the IC amplification.

An invalid result for a clinical sample can be due to PCR inhibition or a failure during the nucleic acid isolation procedure. In such cases, it is recommended to dilute the nucleic acid extract 1:10 (recommended to be done in elution buffer, if possible) for a PCR retest or to repeat the nucleic acid isolation procedure. Note that the dilution of the nucleic acid extract might also lead to a reduction of the target nucleic acid concentration below the limit of detection of the ANCHOR VZV PCR Kit.

9.4.2 ▶ Quantitative Analysis


For a valid run and as a prerequisite for the interpretation of the individual clinical sample results, the following requirements have to be met by the included kit controls:

Channel/Target	VZV	IC	Correlation Coefficient r ²	Slope m
QS1-4 VZV	+	(+) ²	≥0.99	-3.0 to -3.6
NC DNA	-	+	-	-

² QS1 and QS2 VZV are excluded from this rule. The presence of high concentrated artificial nucleic acids in this Standard can result in a competitive inhibition of the IC amplification.

If one of the conditions has failed, the quantitative interpretation of the clinical sample results might be flawed. In such cases, it is recommended to repeat the PCR run.

If all criteria are met, the standard curve generated with QS1-4 VZV of known concentrations can be used to determine the VZV DNA load present in a clinical sample.

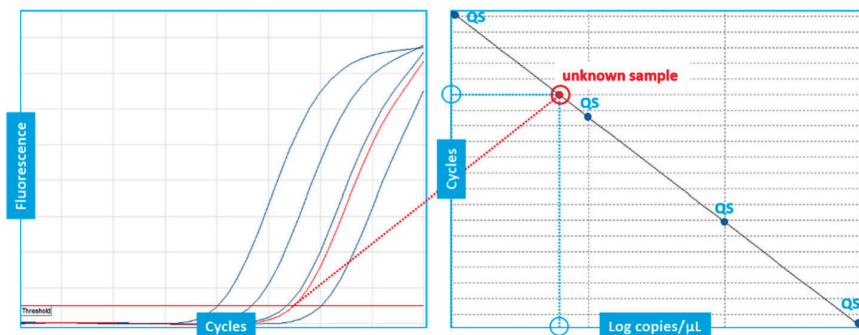

The concentration of any target DNA within a sample eluate will be quantified according to the formula

$$Conc. = 10^{\frac{C_t - b}{m}}$$

where *m* is the slope of the standard curve and *b* the y-intercept.

The results are displayed in copies / μL. To calculate the concentration of VZV DNA in the original clinical sample in copies/mL, the concentration factor of the applied sample preparation system must be considered:

$$Sample \frac{\text{copies}}{\text{mL}} = Eluate \frac{\text{copies}}{\mu\text{L}} \times \frac{\text{Volume Eluate } [\mu\text{L}]}{\text{Volume Sample input } [\text{mL}]}$$

10 ▶ Performance Data

10.1 ▶ Analytical Performance

10.1.1 ▶ Sensitivity

The LOD for the ANCHOR VZV PCR Kit was determined by undertaking a probit analysis on the Rotor-Gene Q platform. A dilution series of different concentration levels for VZV strain Ellen DNA (ATCC / LGC Mat # VR-1367DQ) was used. Each dilution level was tested with overall 24 replicates using 3 different PCR reagent lots across 3 different days, executed by 2 different persons on 2 different instruments.


The LOD value determined on the Rotor-Gene Q was then confirmed or re-evaluated on the other 5 instruments.

Instrument	LOD	Unit
QuantStudio 5	0.25	copies/μL
LightCycler 480 II (Roche)	0.25	copies/μL
cobas z 480 Analyzer	0.25	copies/μL
CFX96	0.25	copies/μL
Rotor-Gene Q	0.25	copies/μL
Mic qPCR	0.50	copies/μL

10.1.2 ▶ Linearity

The linear range of the ANCHOR VZV PCR Kit was determined by testing a dilution series of artificial DNA comprising the VZV PCR target, ranging from 1.00E+07 copies/μL to 1.00E+00 copies/μL. The dilutions were analyzed concentration-dependent with 4-8 replicates. All replicates of one dilution were tested in one PCR run. The linear range was determined with two ANCHOR VZV PCR Kit lots.

The picture below shows a scatter chart of measured concentrations plotted against their nominal concentrations. The correlation of data is described by linear, 2nd and 3rd order polynomial curve fitting.

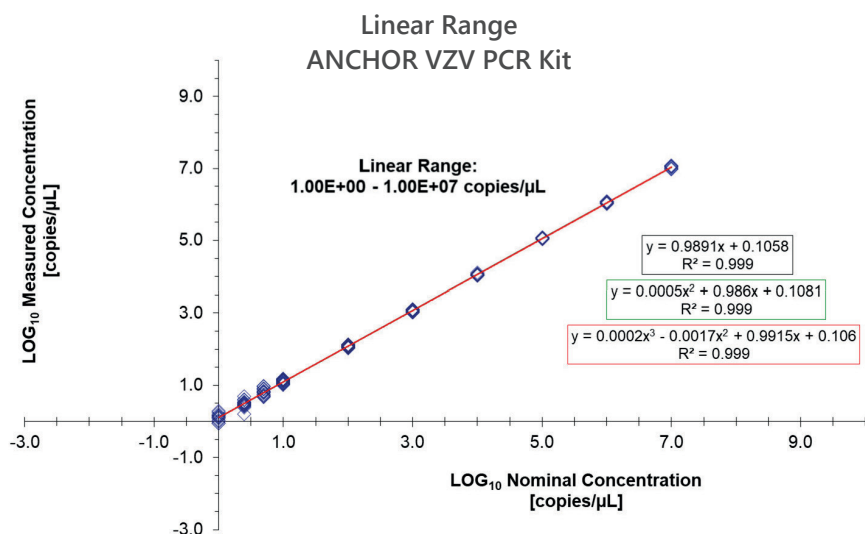

The linear quantification range for the ANCHOR VZV PCR Kit was tested and confirmed to be from at least 1.00E+00 up to 1.00E+07 copies/μL. The Limit of Quantitation (LOQ) is therefore determined to be 1.00E+00 copy/μL.

10.1.3 ▶ Specificity

Triplicates of two different VZV culture strains were tested at a concentration near the 3x LOD of the ANCHOR VZV PCR Kit.

Strain	VZV
VZV strain Ellen	+
VZV strain Webster	+

Nucleic acid of selected pathogens with a concentration of ~5.00E+03 copies/μL (alternative units CFU/μl or TCID50/μL) was added to the PCR reaction and tested in triplicates in the absence or presence of VZV DNA at its 3x LOD and 3x LOQ concentration on the Rotor-Gene Q.

Pathogen	- VZV	3x LOD VZV	3x LOQ VZV $\Delta \text{Log}_{10} \text{ copies}/\mu\text{L}^3$
HSV-1	-	+	0.01
HSV-2	-	+	0.01
BK Virus	-	+	-0.17
Human Cytomegalovirus	-	+	-0.05
Epstein-Barr Virus	-	+	0.02
Hepatitis B Virus	-	+	-0.06
Human Herpesvirus 7	-	+	-0.05
Human Parvovirus B19	-	+	-0.06
Enterovirus 71	-	+	-0.05
West-Nile Virus	-	+	-0.06
<i>Candida albicans</i>	-	+	0.02
<i>Neisseria gonorrhoeae</i>	-	+	-0.01
<i>Gardnerella vaginalis</i>	-	+	-0.02
<i>Clostridium perfringens</i>	-	+	-0.02
<i>Escherichia coli</i>	-	+	-0.06
<i>Salmonella typhimurium</i>	-	+	-0.02

³ In relation to VZV DNA-only control

10.1.4 ▶ Precision

Precision testing was initially performed on the Rotor-Gene Q instrument. For intra-run variability, 3-6 replicates of each sample dilution were tested within one run using one instrument and reagent lot by one operator. For inter-run variability, 3-6 replicates of each sample dilution were tested within overall four runs using two instruments and one reagent lot by two operators across days. For inter-batch variability, 3-5 replicates of each sample dilution were tested within one run using one instrument and three reagent lots by one operator.

QS1 VZV			
Variability	AVE (CT)	SD (CT)	CV (%)
Intra-Run	19.94	0.02	0.09
Inter-Run	20.05	0.08	0.38
Inter-Batch	19.94	0.04	0.22
Total	20.01	0.09	0.43
QS4 VZV			
Variability	AVE (CT)	SD (CT)	CV (%)
Intra-Run	29.86	0.33	1.10
Inter-Run	29.90	0.22	0.75
Inter-Batch	29.89	0.19	0.65
Total	29.90	0.19	0.65
QS VZV LOQ (1 copy/ μL)			
Variability	AVE (CT)	SD (CT)	CV (%)
Intra-Run	32.78	0.37	1.12
Inter-Run	32.90	0.50	1.52
Inter-Batch	32.87	0.47	1.44
Total	32.90	0.50	1.52
ATCC VZV LOQ (1 copy/ μL)			
Variability	AVE (CT)	SD (CT)	CV (%)
Intra-Run	33.09	0.41	1.23
Inter-Run	33.27	0.53	1.60
Inter-Batch	32.94	0.53	1.62
Total	33.14	0.57	1.73

Precision of the ANCHOR VZV PCR Kit in combination with the other instruments was evaluated for intra- and inter-run variability.

10.2. ▶ Clinical Performance

The clinical performance of the ANCHOR VZV PCR Kit for the qualitative and quantitative detection of VZV DNA in human CSF samples and cutaneous/mucocutaneous swabs was evaluated comparatively at 3 different study sites against established VZV routine diagnostic workflows using CE-marked PCR assays as reference standard.

411 prospectively collected specimen were analyzed with the ANCHOR VZV PCR Kit and with the comparator assays to determine their positive percent agreement (PPA) and negative percent agreement (NPA), respectively. Testing was done using the LightCycler 480 II and QuantStudio 5.

ANCHOR VZV PCR Kit	Σ 411	Comparators	
		POS	NEG
	POS	85	5
NEG	4	317	

PPA: 95.5 % NPA: 98.4 %

The clinical performance for human EDTA plasma was evaluated at 2 different study sites against an established VZV routine diagnostic workflow using a CE-marked PCR assay as reference standard.

192 EDTA-plasma samples were analyzed with the ANCHOR VZV PCR Kit and with the comparator assay to determine their positive percent agreement (PPA) and negative percent agreement (NPA), respectively. Testing was done using the Mic qPCR cyclers.

ANCHOR VZV PCR Kit	Σ 192	Comparator	
		POS	NEG
	POS	48	2
NEG	1	141	

PPA: 98.0 % NPA: 98.6 %

11 ▶ Quality Control


In accordance with the implemented ISO 13485-certified Quality Management System, each lot of the ANCHOR VZV PCR Kit is tested against pre-determined specifications to ensure consistent product quality.

12 ▶ Technical Assistance & Contact Information

For any questions, a need for technical assistance or if you identify difficulties using our products do not hesitate to contact us:

phone: +49 40 52 471 62 0

email: support@anchor-diagnostics.com



Grandweg 64
22529 Hamburg | Germany
phone: +49 40 52 471 62 0
www.anchor-diagnostics.com